

Operating Manual

Model 75-810 & 75-810-AR Noble Gas Purifier

75-810-HE: 120 V, 50/60 Hz

75-812-HE: 230 V, 50/60 Hz

75-810-AR: 120 V, 50/60 Hz

75-812-AR: 230 V, 50/60 Hz

October 2024

Rev. 4

**READ INSTRUCTIONS
BEFORE OPERATING**



Contents

Chapter 1 - Introduction.....	9
Chapter 2 - Safety Precautions	11
Chapter 3 - Specifications	13
Chapter 4 - Installation	15
Chapter 5 - Operation.....	17
Chapter 6 - Maintenance & Servicing.....	19
Chapter 7 - Replacement Parts	21
Chapter 8 - Appendix.....	23

DISCLAIMERS

The information in this document is subject to change without notice. This manual could include technical inaccuracies or typographical errors. Changes are made periodically to the information herein; these changes will be incorporated in subsequent revisions of the manual. GOW-MAC® Instrument Co. reserves the right to make improvements and/or changes to the product(s) and/or programs described in this manual at any time and without notice.

All information referred to and/or included in this report is current as of the original issue date of this manual. GOW-MAC® Instrument Co. makes no warranty or representation with respect to the accuracy of the information or with respect to the suitability of the use of such information outside GOW-MAC® Instrument Co., nor does GOW-MAC® Instrument Co. assume responsibility for any injury or damage which may result, directly or indirectly, from the use of such information.

This document contains proprietary information which is protected by copyright. All rights are reserved. No part of the document may be photographed, reproduced, or translated into another language without the prior written consent of GOW-MAC® Instrument Co.

The warranties made by GOW-MAC® Instrument Co. with respect to the product are voided if the product is not used and serviced in accordance with the instructions in this manual.

Please protect yourself and your employees by following these operating instructions. We encourage our customers to write or call for any additional information relative to the use or repair of this instrument.

TRADEMARK AND PATENT INFORMATION

®GOW-MAC is a registered trademark of GOW-MAC Instrument Co.

in the United States and other countries.

Other trademarks used herein are trademarks or registered trademarks of their respective owners.

Swagelok® - is a registered trademark of Crawford Fitting Co.

Parker® - is a registered trademark of Parker Hannifin Corp.

Gyrolok® - is a registered trademark of Hoke, Inc.

LIABILITY Buyer assumes all responsibility for warning and protecting its employees and independent contractors with respect to all hazards to persons and property in any way connected with the Equipment and the use thereof. Seller's liability for any claim of any kind hereunder, whether or not based on contract, tort (including negligence), strict liability, warranty, or any other grounds, shall not exceed the purchase price of the Equipment or the portion of the purchase price attributable to any part or parts of the Equipment in respect to which such claim is made. Seller shall not be liable for any special, indirect, incidental, or consequential damages. Without limiting the generality of the foregoing, Seller shall have no liability with respect to the results obtained by use of the Equipment, whether in terms of product condition, operating cost, general effectiveness, success or failure, or regardless of any statement made in any written proposal submitted by Seller. It is expressly understood that any technical advice furnished by Seller with reference to the Equipment is given gratis and Seller assumes no obligation or liability for the advice given or results obtained, all such advice being given and accepted at Buyer's risk. Each party hereby agrees to indemnify and hold the other party harmless from any actions, lawsuits, demands, claims, losses, expenses, costs, including but not limited to legal fees, and damages arising from the injury, illness or death of the indemnifying party's employees in any way related to the Equipment, whether or not such injury, illness, or death is claimed to have been caused by, resulted from, or was in any way connected with the negligence of the party to be indemnified.

PROPRIETARY INFORMATION Buyer agrees to maintain all proprietary information disclosed by Seller, including such proprietary information obtainable upon examination of the Equipment, in confidence and to refrain from any disclosure thereof to any third party (including any affiliate of Buyer), for any purpose, without the prior written consent of Seller. Buyer agrees to use said proprietary information solely for purposes of maintaining and operating the Equipment, and to refrain from any use thereof to design, construct, have constructed and/or operate any duplication or modification of the Equipment, or from any other use thereof, without the prior written consent of Seller.

Models Affected

75-810-HE

75-812-HE

75-810-AR

75-812-AR

Warranty

ALL INSTRUMENTS SOLD BY GOW-MAC® INSTRUMENT CO. ARE WARRANTED FOR A PERIOD OF ONE YEAR AGAINST DEFECTS IN MATERIALS AND WORKMANSHIP. THE TERMS OF THIS WARRANTY ARE AS FOLLOWS:

1. **The warranty period begins with the shipping date of the equipment to the original purchaser.**
2. Certain parts such as batteries, fuses, glass accessories, septa, columns, etc., are expendable in normal use, and their service life is unpredictable. Such items are not covered by this warranty.
3. Filaments of thermal conductivity detectors are not covered by this warranty.
4. Hydrogen Palladium Tubes are not covered by this warranty.
5. All requests for service or repair under this warranty must be received within the warranty period by GOW-MAC® or its authorized representative. All repairs are made at GOW-MAC plants or at the office of authorized representatives.
6. All repairs, adjustments, and other services under this warranty shall be performed free of charge to the purchaser. However, warranty service and repairs shall be limited to equipment malfunctions which, in the opinion of GOW-MAC®, are due or traceable to defects in original materials or workmanship. Instrument malfunctions caused by abuse or neglect of the equipment are expressly not covered by this warranty.
7. Instrument parts which have been repaired or replaced during the warranty period are themselves warranted only for the remaining unexpired portion of the original one-year warranty.
8. Repairs, adjustments, and service performed after expiration of the one-year warranty period shall be charged to the purchaser at the then current prices for parts, labor, and transportation.
9. This warranty attaches to the equipment itself and is not limited to the original purchaser. Unexpired portions of the warranty are thus transferable to subsequent owners.
10. GOW-MAC® expressly disclaims any liability to users of its products for consequential damages of any kind arising out of or connected with the use of its products.
11. Except as stated in Sections 1 through 8 above, GOW-MAC® makes no warranty, expressed or implied (either in fact or by operation of law), statutory or otherwise; and, except as stated in Sections 1 through 8 above, GOW-MAC® shall have no liability under any warranty, expressed or implied (either in fact or by operation of law), statutory or otherwise.
12. Statements made by any person, including representatives of GOW-MAC® which are inconsistent or in conflict with the terms of this warranty shall not be binding upon GOW-MAC® unless reduced to writing and approved by an officer of the Company.
13. This warranty shall be governed by the laws of the Commonwealth of Pennsylvania.

7/8/24
kj

Noble Gas Purifier

Models 75-810-HE/75-812-HE & 75-810-AR/75-812-AR

1 Introduction

The 75-810 series of purifiers are designed for the purification of noble gas and under no circumstances shall they be utilized for the purification of hydrogen, nitrogen, oxygen, air or other reactive gases. Please read and understand the following manual and documents prior to beginning the installation of the 75-810. If there is anything not understood, please call for clarification prior to operation. 75-810-HE/AR designates models for 120 VAC service and 75-812-HE/AR for 230 VAC service. All versions may be generically referred to as 75-810 throughout this manual where appropriate.

The GOW-MAC 75-810 series are point-of-use gas purifiers that remove impurities (H₂O, O₂, CO, CO₂, H₂, N₂, CH₄) from ultra-high purity (99.999%) argon or helium. The bench-top configuration is compact with ¼ inch VCR connections for gas in and out on the top panel. The getter material is heated to about 400 °C when the power switch is ON and illuminated. The heated cartridge is wrapped in insulation that is easily removed for service. A second stage getter for hydrogen removed is directly downstream from the first stage. The hydrogen trapping is more efficient when colder so that section of the cartridge is wrapped in a heatsink to transfer heat away from the cartridge. The final feature of the flow path is an integral 0.003 micron particle filter. The 75-810 purifiers are factory-conditioned for optimal performance with helium or argon (denoted in the part number by –HE and –AR).

UltraPure™ is a registered trademark of UltraPure Systems Inc.

2 Safety Precautions



SAFETY WARNINGS



WARNING

This purifier is intended for the purification of NOBLE* gas only. Under NO circumstances should it be used for the purification of hydrogen, nitrogen, oxygen, air, or reactive gases.

Failure to comply can result in personal injury and/or mechanical damage to purifier and all warranties shall be void.

*Noble gas refers to Ar, He, Ne, Kr, Xe.

WARNING

This equipment processes gas using electrical equipment. Serious injury can result if maintenance is performed with the power on. Always shut power off at the facility circuit breaker before maintenance is to be performed. In addition, lock out the associated circuit breaker in accordance with local safety directives to prevent an advertent operation by facility personnel until maintenance has been completed and all personnel are clear of the machinery.

WARNING

This equipment processes gas at high temperatures. Serious burns can result. If maintenance is to be performed, allow unit to cool to room temperature prior to any maintenance or service.

WARNING

Electric shock hazard potential exists inside the unit. Take the necessary safety precautions to avoid touching exposed terminals and wiring. Failure to comply can result in death, personal injury or damage to the purifier.

WARNING

MAXIMUM VESSEL OPERATING PRESSURE: 250 PSIG

SAFETY CAUTIONS

CAUTION

All gas lines and connections **MUST** be leak-checked prior to operation of the unit in order to ensure the integrity of the system and to prevent any exposure of the getter bed to atmosphere. The getter material in the purifier may be destroyed if exposed to atmosphere while its temperature is above 150 °C.

CAUTION

If a gas line should become disconnected during normal operation, the purifier must be shut down and all inlet/outlet valves should be closed in order to isolate the unit from the facility lines. This will limit the exposure of the getter bed to atmosphere while it is in excess of 150 °C. Do not restart the purifier until temperature has cooled to below 150 °C and all gas lines have been reconnected/repared and certified. Failure to comply can result in personal injury or damage to the purifier.

CAUTION

The purity guarantees are void if installation is other than that approved by GOW-MAC Instrument Company

CAUTION

During heated operation, this unit **MUST** be pressurized with noble gas and isolated from any exposure to atmosphere or the getter bed will be destroyed.

3 75-810 Specifications

Gases Purified	He, Ne, Ar, Kr, Xe
*Impurities Removed:	H ₂ O, H ₂ , O ₂ , N ₂ , CO, CO ₂ , CH ₄
Impurities Not Removed:	He, Ne, Ar, Kr, Xe
Operating Temperature:	400 °C ± 25 °C
Temperature Sensor:	K-Type thermocouple is integrated in the heater, monitor the cartridge temperature by connection with a flat pin connector to the receptacle on the top panel
Maximum Recommended Operating Pressure:	17.0 atm (250 psig)
Suggested Maximum Flow Rates (ccpm):	Model 75-810: 1500
**Gas Connections:	1/4" VCR® Male
Leak to Atmosphere	<2 X 10 ¹⁰ atm-cc/sec helium
***Lifetime Purifying He or Ar:	75-810: 1 yr. @ 200 ccpm
Power Requirements:	75-810: 80 Watts, 120 VAC 75-812: 80 Watts, 230 VAC
Circuit Breaker	In power switch, fast acting, 1A rating
Weight (net):	3.5 lbs.
Dimensions:	5"D x 4"W x 10"H

* Each impurity removed to < 10 ppb based on 10 ppm total inlet impurities at suggested maximum flow rate

** VCR® is a registered trademark of Swagelok Corporation


*** Lifetime based on suggested maximum flow rates; a higher flow rate will proportionally decrease the lifetime while a lower flow rate will increase the lifetime. The lifetime is rates at 10 ppm total inlet impurities; higher or lower inlet impurity levels will decrease or increase the lifetime proportionally. The purifier bed is considered an expendable item. System leaks, poor quality gas, and improper handling will adversely affect its useful life.

4 Installation


Locate the 75-810 on a table top with the rubber feet on the surface. In this position, the gas in and out connections are on top and the purifier cartridge is in the correct vertical orientation which reduces gas channeling through the getter material.

Connect the 75-810 fitting marked GAS IN to the source of carrier helium or argon. A diaphragm shut-off valve in the supply line will facilitate servicing the 75-810. Recommended tubing specification is 1/8 inch OD X 0.028 wall, 316L stainless steel, cleaned or electropolished. Orbital butt weld a 1/4 inch VCR® gland including a female nut for connection to the 75-810. Test any new weld to verify there is no leak. Likewise prepare a tube to connect to the GAS OUT fitting. Connect the 75-810 GAS OUT to the CARRIER IN connection on the gas chromatograph or ZERO GAS IN connection on an analyzer.


The flat pin receptacle on the top panel allows monitoring of the cartridge temperature. For usual operation, monitoring is not necessary because the heater should operate at optimum temperature when the 75-810 is powered on. It is during transitions to start-up and shut-down that knowing the temperature is important, especially the 150 °C point that is referred to throughout this manual. Use a flat pin thermocouple connector (not provided) and K thermocouple leads connected to a suitable meter to monitor 75-810 temperature.

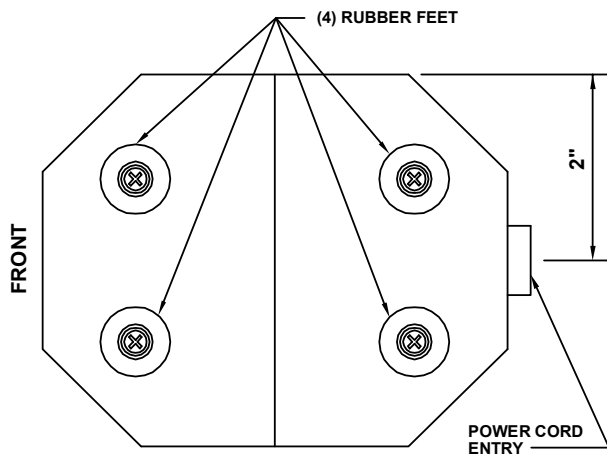


BOTTOM VIEW

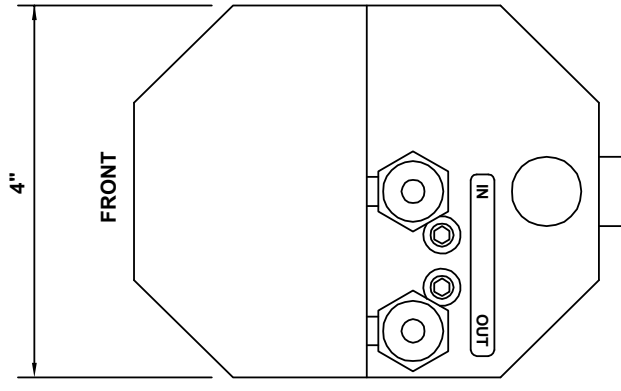

TOP VIEW

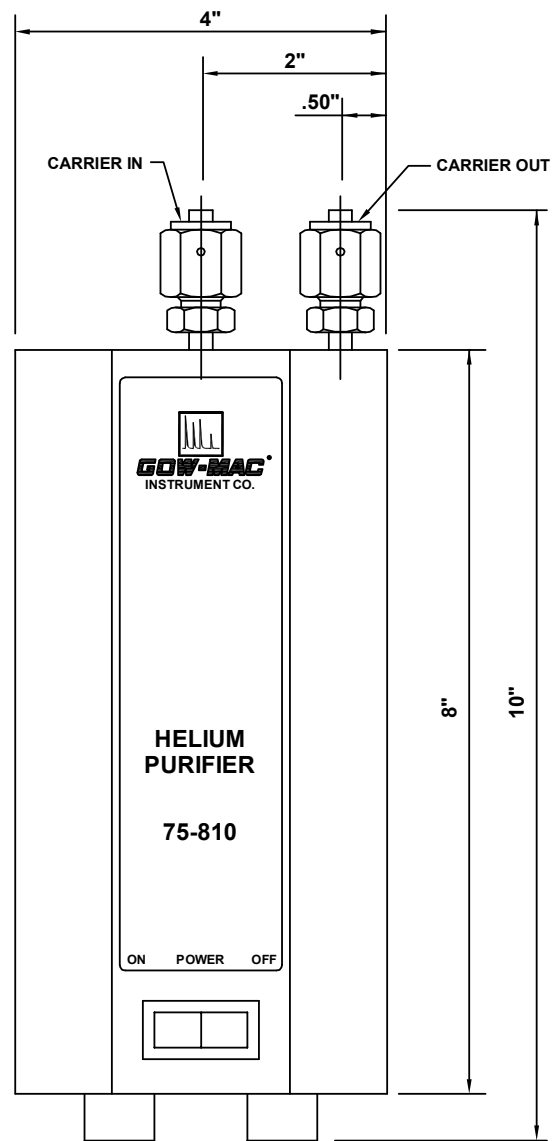

FRONT VIEW

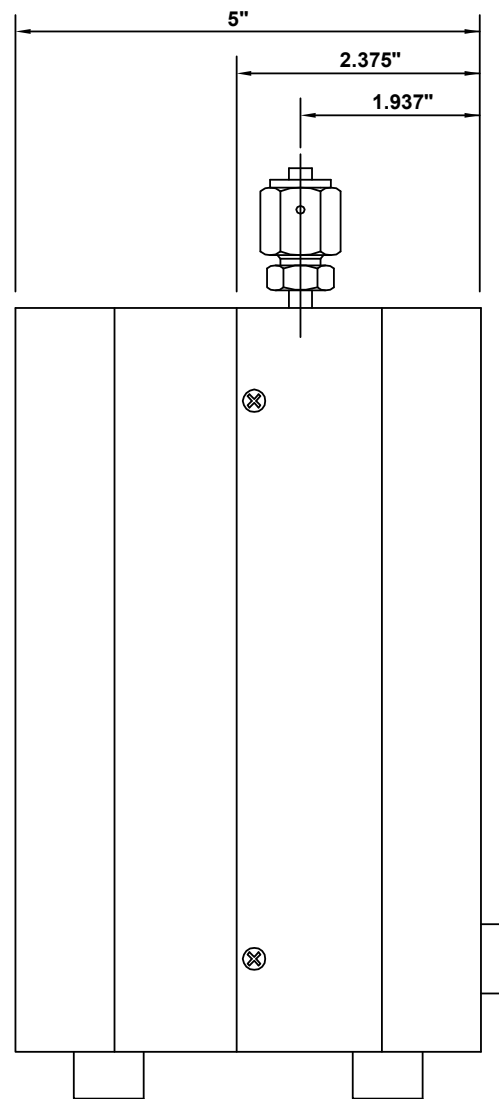

SIDE VIEW

5 Operation

Start Up

The purifier should be purged with an inert gas (helium if -HE or argon if -AR model, minimum purity 99.99%) for at least 10 minutes before powering on. Apply continuous gas flow of 50 to 200 ccpm before and during initial activation. After the 10 minute purge period, switch on power to the 75-810. The heater is selected to heat the purifier to about 400 °C. At this temperature, the purifier material will take 3 hours to fully activate. After this activation period, the purifier is ready to operate at the desired flowrate.

CAUTION

IF THE 75-810 SUPPLY OR VENT LINE IS ACCIDENTALLY VENTED TO ATMOSPHERE, ASSUME AIR HAS ENTERED THE PURIFIER. IMMEDIATELY SWITCH OFF POWER AND FLOW HELIUM OR ARGON THROUGH THE PURIFIER AT 50 TO 200 CCPM TO PURGE OUT ANY AIR. EXPOSURE OF THE GETTER MATERIAL TO OXYGEN WHEN IT IS ABOVE 150 °C WILL DESTROY THE MATERIAL AND MAY INITIATE AN EXOTHERMIC REACTION.

Examples of the performance of the 75-810 for helium and argon gases are in the Appendix.

Shutdown

If the gas line containing the 75-810 is to be vented to air, for example during purifier replacement, then the purifier must be at room temperature before venting to air. If the purifier is hot, switch off power, maintain gas flow and wait 3 hours to allow the purifier to reach room temperature.

6 Maintenance & Servicing

Purifier Lifetime

In order to maintain proper purification efficiency, do not exceed estimated lifetime of the purifier cartridge. The estimated lifetime (first impurity breakthrough) is 1 year at 400 °C operating temperature, 150 ccpm flowrate, and inlet gas purity of 99.999%. First breakthrough of H₂ or O₂ at these conditions should be after about 4 years. Lifetime is inversely proportional to the total inlet impurity level and to the average flow rate.

The getter material in 75-810 models cannot be regenerated so the cartridge must be changed. In the unlikely event of H₂ or O₂ breakthrough, the hydrogen removal stage can be regenerated in the field.

Hydrogen stage regeneration

- Power off the 75-810 and allow 3 hours to cool while maintaining minimum 50 ccpm inert gas flow through the cartridge. Monitor the temperature using the K thermocouple on the unit. Ensure cartridge temperature is below 150 °C before turning off gas flow. Keep all gas connections intact if possible to prevent ingress of air.
- Switch off power on the 75-810 and UNPLUG THE POWER CORD.
- Open the case
- Loosen the hose clamp on the heatsink which is on the hydrogen removal stage. Slide the heatsink away from the cartridge.
- Move the heater and insulation from the first stage to the hydrogen stage and re-tighten both.
- Check integrity of wire connections inside the case
- Follow the steps for initial activation in order to regenerate the hydrogen stage. Refer to Section 5 Operation/Start Up for activation procedure.
- After regeneration, replace heater, insulation, and heatsink to their original locations, check wire connections, and close the case.

Replacing the cartridge and/or heater

- Power off the 75-810 and allow 3 hours to cool while maintaining minimum 50 ccpm inert gas flow through the cartridge. Monitor the temperature using the K thermocouple on the unit. Ensure cartridge temperature is below 150 °C before turning off gas flow. Keep all gas connections intact if possible to prevent ingress of air.
- Switch off power on the 75-810 and UNPLUG THE POWER CORD.
- Open the case
- Loosen the hose clamp on the heatsink which is on the hydrogen removal stage. Slide the heatsink away from the cartridge. Retain heatsink for re-assembly.

- Remove the insulation and retain for re-assembly
- Remove the heater and retain for re-assembly unless also replacing the heater
- With one each 5/8 inch and 3/4 inch open end wrenches, undo the VCR® connections on the cartridge and remove the two gaskets, which should be discarded.
- Insert the new cartridge, TAKING CARE TO PLACE THE FIRST STAGE CLOSEST TO THE GAS IN FITTING. Use new VCR® gaskets provided with the replacement cartridge. Assemble the VCR® nut finger tight and then use the wrenches to tighten a further quarter-turn.
- Replace heater, insulation, and second stage heatsink. Tighten all hardware and secure insulation and heatsink on the first and second stages respectively
- Check integrity of wire connections inside the case and close the case
- Follow the steps for initial activation. Refer to Section 5 Operation/Start Up for activation procedure.

Waste Disposal

This procedure is for the purifier cartridges in all models 75-810.

If the purifier is used, then the getter material inside the purifier is already in a non-reactive state, (i.e. will not react with air).

If the material is still in a reactive state (i.e. the purifier is not completely "used up"), it still will not sustain combustion in air except at temperatures over 350 °C, and with a continued exposure to air.

The operator should place a VCR® cap on the inlet and outlet fittings for sufficient precaution before disposal. It is then acceptable to deposit in an approved landfill, in accordance with local, state and/or federal regulations. When disposed of in this manner, the waste poses no known environmental problems.


7 Replacement Parts

<u>Part No.</u>	<u>Description</u>
124-240-F	Heater, 115 VAC, 80 W (includes integral K thermocouple)
124-241-F	Heater, 230 VAC, 80 W (includes integral K thermocouple)
180-1000-HE	Purifier cartridge for helium, 1/4" VCR® male connections. Includes hydrogen removed stage and internal 0.003 micron filter and two (2) VCR® gaskets. Does not include insulation or heatsink.
180-1000-AR	Purifier cartridge for argon, 1/4" VCR® male connections. Includes hydrogen removed stage and internal 0.003 micron filter and two (2) VCR® gaskets. Does not include insulation or heatsink.

8 Appendix

Summary of Helium Purifier Performance in Removing Impurities

Instrument : GOW- MAC Series 200 GC
 Detector : DID
 Detector Temperature : 35°C
 Detector Flow : 10 ml/min
 Column : 4.5' x 1.8" Molecular Sieve 13X
 Oven Temperature : 50°C
 Sample Gas : 2 ppm standard atmospheric gases in Helium
 Sample Flow : 60 ml/min
 Carrier Gas : Helium
 Carrier Flow : 30 ml/min
 Purifier Operating Temperature : 400°C (Factory pre- set)

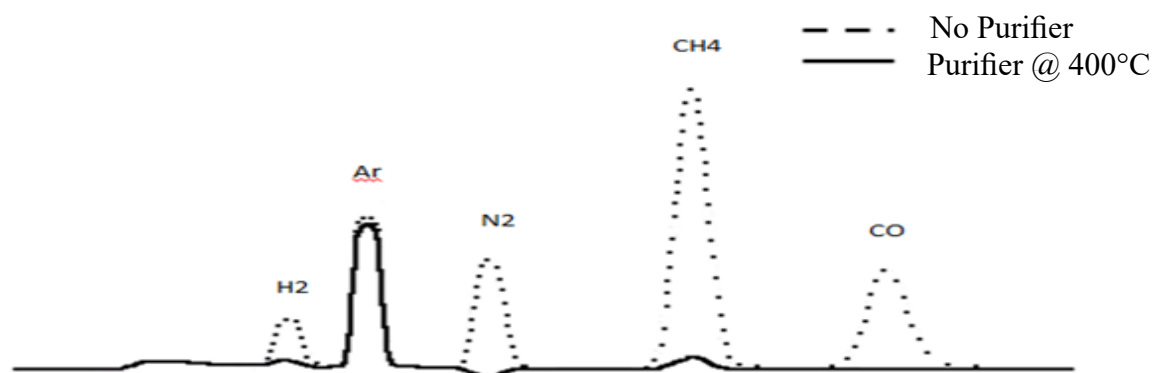

Impurities	Responses (mV.s)	Concentration (ppm)
H2	13.795	0.093
Ar	962.303	1.906
N2	68.516	0.189 (- ve peak)
CH4	92.381	0.085
CO	0.000	0.000


Table 1: Remaining Concentration of Impurities with Helium Purifier at 400°C

Key Findings:

1. CO is totally removed.
2. N2 peak is negative: N2 is removed by purifier so less N2 remains in sample line compared to in carrier gas.
3. Other peaks (except for Argon) are reduced to ppb level.

Summary of Argon Purifier Performance in Removing Impurities

Instrument : GOW- MAC Series AR710 GC
 Detector : HFADD
 Detector Current : 47 mA
 Column : 10' x 1/8" Molecular Sieve 13X
 Oven Temperature : 80°C
 Sample Gas : 2 ppm atmospheric gases in Argon
 Sample Flow : 60 ml/min
 Carrier Gas : Argon
 Carrier Flow : 40 ml/min
 Purifier Operating Temperature : 400°C (Factory pre- set)

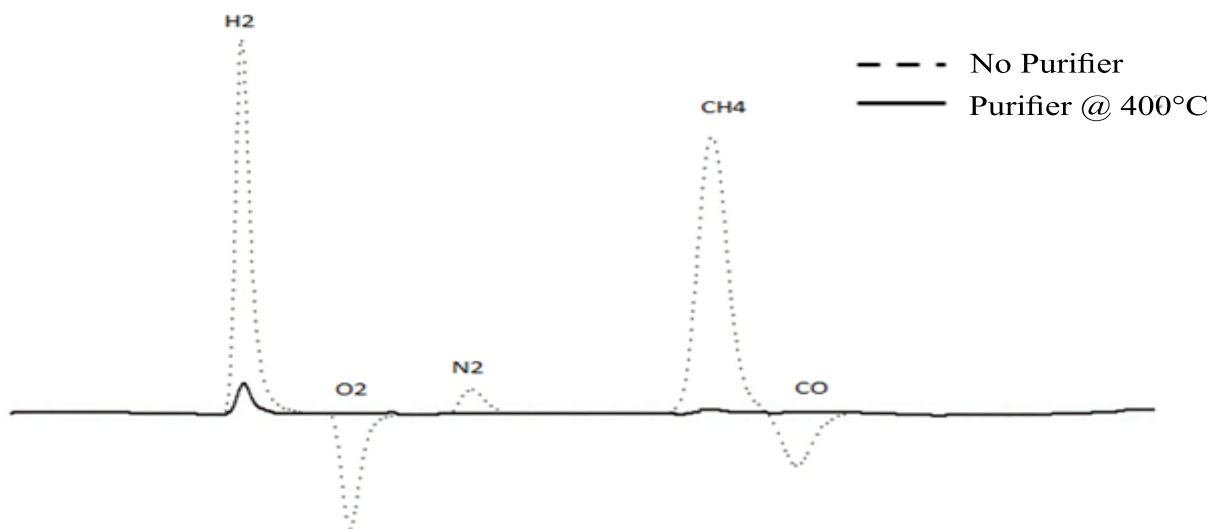

Impurities	Responses (mV.s)	Concentration (ppm)
H2	259.943	0.215
O2	0.000	0.000
N2	0.000	0.000
CH4	58.359	0.034
CO	0.000	0.000

Table 2: Remaining Concentration of Impurities with Argon Purifier at 400°C

Key Findings:

1. O2, N2, and CO are totally removed.
2. H2 and CH4 are reduced to ppb level.